

Human MDA-modified oxidized low-density lipoprotein ELISA Kit | MDA-oxLDL elisa kit

Human MDA-modified oxidized low-density lipoprotein ELISA Kit

CATALOG #
AAA247193

REACTIVITY
Human


PRODUCT SYNONYMS

MDA-modified oxidized low-density lipoprotein; Human MDA-modified oxidized low-density lipoprotein ELISA Kit; MDA-oxLDL elisa kit

PRODUCT SPECIFICATIONS

Reactivity	Human
Specificity	This assay has high sensitivity and excellent specificity for detection of MDA-oxLDL. No significant cross-reactivity or interference between MDA-oxLDL and analogues was observed. NOTE: Limited by current skills and knowledge, it is impossible for us to complete the cross-reactivity detection between MDA-oxLDL and all the analogues, therefore, cross reaction may still exist in some cases.
Assay Type	Quantitative Competitive
Samples	Serum, plasma, cell culture supernatants, body fluid and tissue homogenate
Sensitivity	1.0 ?g/mL

IMAGES

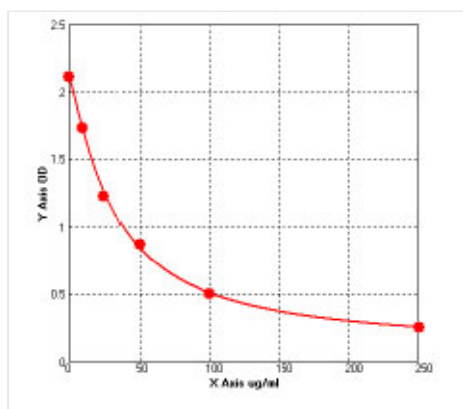

Standard Curve (Sample)

ADDITIONAL INFORMATION

Related Product Information for MDA-oxLDL elisa kit	Principle of the Assay: MDA-oxLDL ELISA kit applies the competitive enzyme immunoassay technique utilizing a polyclonal anti-MDA-oxLDL antibody and an MDA-oxLDL-HRP conjugate. The assay sample and buffer are incubated together with MDA-oxLDL-HRP conjugate in pre-coated plate for one hour. After the incubation period, the wells are decanted and washed five times. The wells are then incubated with a substrate for HRP enzyme. The product of the enzyme-substrate reaction forms a blue colored complex. Finally, a stop solution is added to stop the reaction, which will then turn the solution yellow. The intensity of color is measured spectrophotometrically at 450nm in a microplate reader. The intensity of the color is inversely proportional to the MDA-oxLDL concentration since MDA-oxLDL from samples and MDA-oxLDL-HRP conjugate compete for the anti-MDA-oxLDL antibody binding site. Since the number of sites is limited, as more sites are occupied by MDA-oxLDL from the sample, fewer sites are left to bind MDA-oxLDL-HRP conjugate. A standard curve is plotted relating the intensity of the color (O.D.) to the concentration of standards. The MDA-oxLDL concentration in each sample is interpolated from this standard curve. Intended Uses: This MDA-oxLDL ELISA kit is a 1.5 hour solid-phase ELISA designed for the quantitative determination of Human MDA-oxLDL. This ELISA kit for research use only, not for therapeutic or test applications!
---	---

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Small volumes of product may become entrapped in the seal of the vial during shipment and storage; if necessary, briefly centrifuge the vial on a tabletop centrifuge to dislodge any liquid in the cap.

AAA Biotech | Tel: +1 (619) 604-9440 | Fax: +1 (619) 604-9441 | contact@aaabiotech.com
Online datasheet: <https://www.aaabiotech.com/mda-oxldl-human-elisa-kits/mda-modified-oxidized-low-density-lipoprotein/247193>